


Titan Workstation User Manual

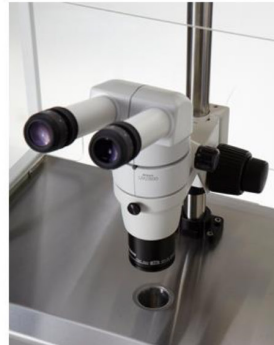

UK
CA

origio,
'S

INDEX





How To Use This Manual.....	3
Introduction.....	4
Intended Purpose	4
SAFETY INSTRUCTIONS.....	5
Before operation of the workstation.....	5
SYMBOLS ON THE EQUIPMENT	6
INSTALLATION	7
Device Placement.....	7
AIR FLOW WORKING PRINCIPLE.....	8
CONTROL PANEL.....	9
GENERAL OPERATING PROCEDURES	10
Connecting the power cord	10
Switching the Fans ON / OFF at Normal Speed	10
Switching the Fans ON / OFF at Reduced Speed.....	10
Alarm	10
Internal Light.....	11
UV Light.....	11
Working Heated Surface	11
CONTROL & PROGRAMMING.....	12
Overview of the Control Panel Menu.....	13
General air flow information & counter	13
Adjusting the level intensity of the internal light.....	14
Programming and Controlling the UV light timer	14
Programming Time and Date	17
Display Mode Functions	20
HEATED SURFACE	22
Operational Characteristics	22
Temperature Controller.....	23
User Setup	24
Accessing the parameters and information menu	24
Resetting the THI and TLO recordings.....	24
Channel 1 set point	24
Standby	25
Keypad lock.....	25
Operating the heated areas.....	25
Normal Operation	25
Checking the temperature	25
TROUBLESHOOTING Your Workstation	26
TECHNICAL SPECIFICATIONS.....	30
SPARE PARTS.....	31
OPERATING THE STEREO MICROSCOPE HEATED GLASS AND LIGHT SOURCE CONTROLLER.....	32
OPERATING THE LCD MONITOR	37
WARRANTY AND LIABILITY	38
CUSTOMER SERVICE CONTACT INFORMATION	39

HOW TO USE THIS MANUAL

Warning, Cautions and important Notes

Throughout this manual, blocks of text may be accompanied with a pictogram. These blocks are WARNINGS, CAUTIONS, and IMPORTANT NOTES and they are used as follows:

Symbols used in this Manual:

	NOTE Used to direct attention to a special item.
	WARNING
	DANGER UV light radiation hazard. Use only with shielding in place. Protect eyes and skin from exposure to UV light.
	FURTHER INFORMATION Further information is provided in other sections or manuals.

INTRODUCTION

You are now in possession of a high quality microprocessor-controlled TITAN workstation and it is designed to provide:

- Protection of the processed product against particle /microbiological contamination
- Heating control of the heated work area for sample handling
- Gassing and Humidification control (Optional)
- Heating control of the light opening for morphology study under microscopy (Optional)

This user manual covers the following models:

- TITAN IVF
- TITAN LAF

The TITAN workstation has a built-in microprocessor controller featuring:

- LCD display indicating fan and alarm status.
- Air velocity sensors
- Clock (7 days) and hour-counter.
- Pre-setting of automatic start-up and UV timer.
- Alarm for any deviation from safety conditions.

Furthermore, the TITAN workstation has the following characteristics:

- Negative pressure plenum for highest sample safety.
- Adjustable fan speeds.
- Work chamber with tabletop in stainless steel (AISI 304).

INTENDED PURPOSE

To reduce Volatile Organic Compounds (VOCs), Chemical Air Contaminants (CACs) and other particulate contaminants from air circulating in a laminar flow hood where Assisted Reproductive Technology (ART) procedures are conducted.

SAFETY INSTRUCTIONS



To avoid unintended or improper operation of the workstation, please read this manual carefully

Before operation of the workstation

Before operating your workstation, please note the following:

	The work chamber is to be carefully cleaned and/or disinfected. Use only hydrogen peroxide (H ₂ O ₂ Solutions) or products suitable to be used in an IVF lab. NEVER use ammonia or chlorinated cleaners. It is recommended to use special lint-free wipes.
	To ensure that the working area is clean and sterile the workstation fan must be run at normal speed for at least 30 minutes prior to working inside the Workstation.
	Objects and instruments must be carefully cleaned and/or disinfected before bringing them into the work chamber.
	Necessary instruments for use during work must be placed within reach to avoid unnecessary movement inside the Workstation.
	For reliable operation it is important that the air-flow conditions are as unobstructed as much as possible. Therefore, never overload the work chamber.
	Put on necessary personal clothing for reducing particle emission from operator (i.e. gloves, masks and general clean room clothing). Special attention should be given to hands and lower parts of the arms, as these are the parts of the operator most likely to emit particles near the product.
	All work in the workstation must be performed with slow movements. Rapid arm movements in the chamber may cause slipstreams, which will draw contaminated air into the work chamber.
	Transport of possibly contaminated material may create airflows which can contaminate the product.
	The safety cabinet must not be used for working with materials which can cause allergic reactions, or any harm to the health of the operator or the personnel. Attention is drawn to the risk assessment requirements of the Control of Substances Hazardous to Health (COSHH) Regulations 1999. (UK)
	The cabinet is not suitable for HIGH-RISK biological agents. HIGH RISK biological agents include all etiologic agents designated Class 4 by CDC, and oncogenic viruses classed high risk by NCI. (USA)
	Never operate the workstation cabinets if the fan compartment cover is removed. If this cover is removed, the cabinet will give no protection of the operator or the environment and the fan will run with openly rotating blades.
	The workstation will not provide any protection for operator or environment against harmful gases or vapors.

SYMBOLS ON THE EQUIPMENT

	Caution – Consult this manual for safety precautions
	Caution - High voltage. Possibility of electric shock.
	Protective Earth Symbol
	Connection for Heated glass control
	Connection for 24V Power Inlet and 24V Power outlet
	Connection for Microscope lamp LS 112 or LS114
	LABORATORY EQUIPMENT WITH RESPECT TO ELECTRICAL SHOCK, FIRE, AND MECHANICAL HAZARDS ONLY IN ACCORDANCE WITH UL 61010-1 (2012), IEC 61010-1 (2010) A (2016) AND CAN/CSA C22.2 NO. 61010.1 (2012)

INSTALLATION




Please see the installation manual


Device Placement

The device should be placed on a level secure surface, away from heaters, coolers and air-conditioning outlets.


The device may only be operated at temperatures ranging between 15 °C and 35°C, with a maximum 80% relative humidity, and at normal air pressure.

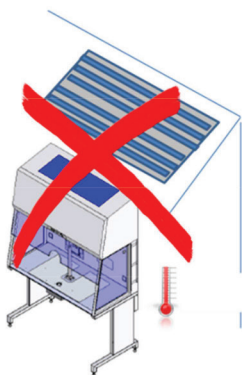

Do not place under a HVAC outlet

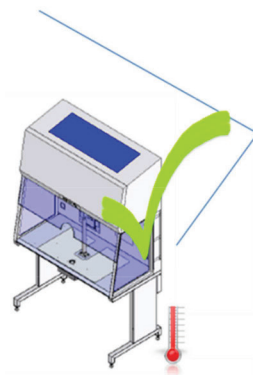

AIR FLOW WORKING PRINCIPLE

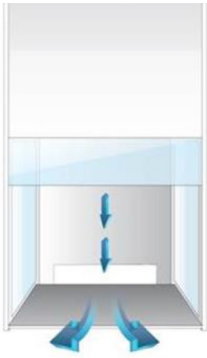


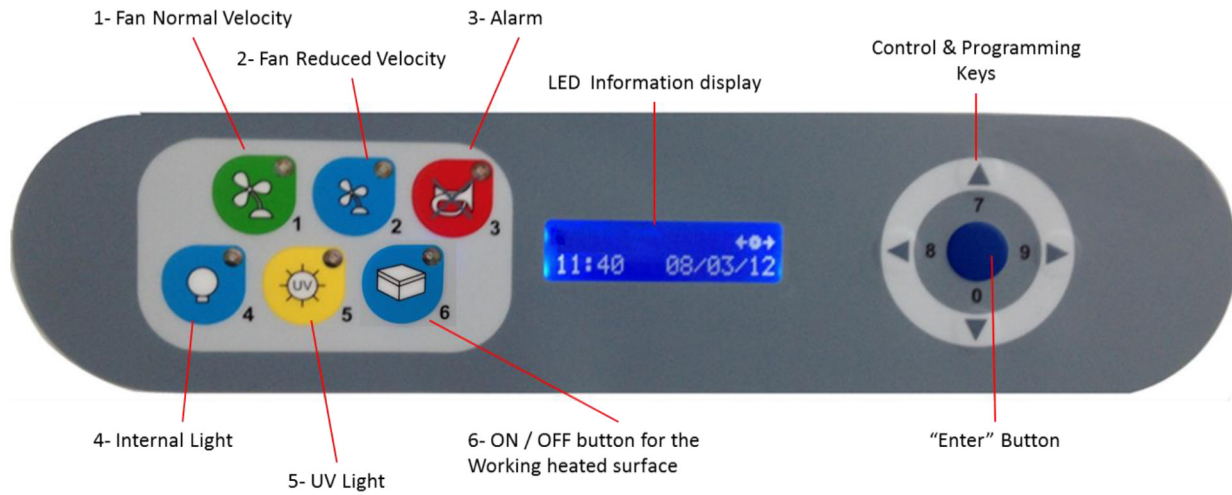
The vertical clean air cabinet is a turbulence-free (laminar) vertical displacement flow of clean air in the work chamber protecting the product against particle contamination.

Filters: The TITAN workstation main filter is a high-efficiency HEPA filter class (H14) and the pre-filter of TITAN is EU-3 type to capture dust particles for increased lifetime of the HEPA filter.

Air velocity monitoring: The turbulence-free vertical flow can be monitored by means of an air velocity sensor. Any deviation from safe conditions will be indicated visually and acoustically.


CONTROL PANEL

During normal use, the LED display shows the time and the day and the “Control and programming keys”  to navigate through the menu program. The numbers 0 to 9 in the control and programming keys are for programming purposes.



GENERAL OPERATING PROCEDURES

Connecting the power cord

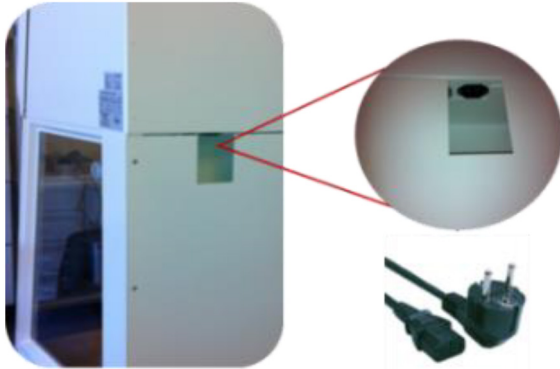

Connect the power cord to the mains power inlet. The power inlet is located at the back of the workstation. The power outlet must be grounded.

As soon as the device is connected an audible alarm will be activated, an LED light will turn on and a message with POWER UP ERROR will be activated on the control panel.

Press the “enter” button to switch off the alarm and to return to safe mode.



Please see the installation manual for further information.

Switching the Fans ON / OFF at Normal Speed



Press the “1- Fan Velocity” button to turn the fans ON. When activated a small green light on top of the button will switch on.



Press the “1- Fan Velocity Button” to turn the fans OFF. When activated the small light on top of the button will be OFF.




To prevent any accidental switching on or off of the fan, the buttons for normal and reduced velocity must be activated for at least 15 seconds before they take effect.



DO NOT WORK IN THE WORK SPACE AREA WHEN THE FANS ARE SWITCHED OFF

Switching the Fans ON / OFF at Reduced Speed



Press the “2- Fan Reduced Velocity” button to turn the fans ON. When activated a small blue light on top of the button will switch on.




Press the “2- Fan Velocity Reduced Button” to turn the fans OFF. When activated the small light on top of the button will be OFF.



When turning ON the reduced speed velocity, the internal light will turn off to alert the user. The internal light can be switched on again if needed.

Alarm



When an alarm is activated an audible acoustic signal is activated. On the control panel a small red light is activated on the Alarm button. Press the Alarm Button to mute the acoustic alarm signal.



The error causing the alarm will be explained on the LED display.



When the error has been fixed the audible alarm and the small red light are switched off.



MUTING THE ACOUSTIC SIGNAL WILL NOT SOLVE THE PROBLEM THAT CAUSED THE ERROR

Internal Light



To switch ON the illumination light of the work chamber, press the “4-Internal Light” button. When activated, a small blue light on top of the button will switch on.



To switch OFF the illumination light of the work chamber, press the “4-Internal Light” button again. The small light on top of the button will be OFF.




To adjust the light intensity, refer to the section “Adjusting the level intensity of the internal light”.

UV Light



The UV light and UV light timer are optional features.



For increased safety against unintended UV radiation which will harm eyes and skin, use the timer to start the UV decontamination when no personnel is present in the room where the workstation is located. Use the front shield cover (Optional) to contain the radiation



To program the UV light time, refer to the section “Programming and Controlling the UV light timer”.



To switch OFF the illumination light of the work chamber, press the “4-Internal Light” button again. The small light on top of the button will be OFF.




To switch ON the UV light for decontaminating the work chamber, press the “5- UV Light” button. When activated a small yellow light on top of the button will switch on


Working Heated Surface



To operate the heated work area, refer to the section “Heated Surface”.










To switch ON the ORIGIO Light Source and the working heated surface (s), press the button. When activated a small blue light on top of the button will switch on. This button simultaneously activates the working heated surface. (Note this feature is not available on the FORTUNA ICSI models)



To switch OFF the working heated surface (s), press the button again. The small light on top of the button will be switched OFF.


CONTROL & PROGRAMMING

This section describes how to access the different menus and how to control and to program some the features offered with your workstation. The Control & Programming menu of your workstation contains the following:

-  Standard display
-  Adjusting the intensity of the internal light
-  Programming and controlling the UV light timer
-  Setting the internal clock
-  Adjusting display settings
-  Programming and controlling the automatic start and shut-off of the fan
-  Entering the service mode

Overview of the Control Panel Menu

CONTROL PANEL MENU

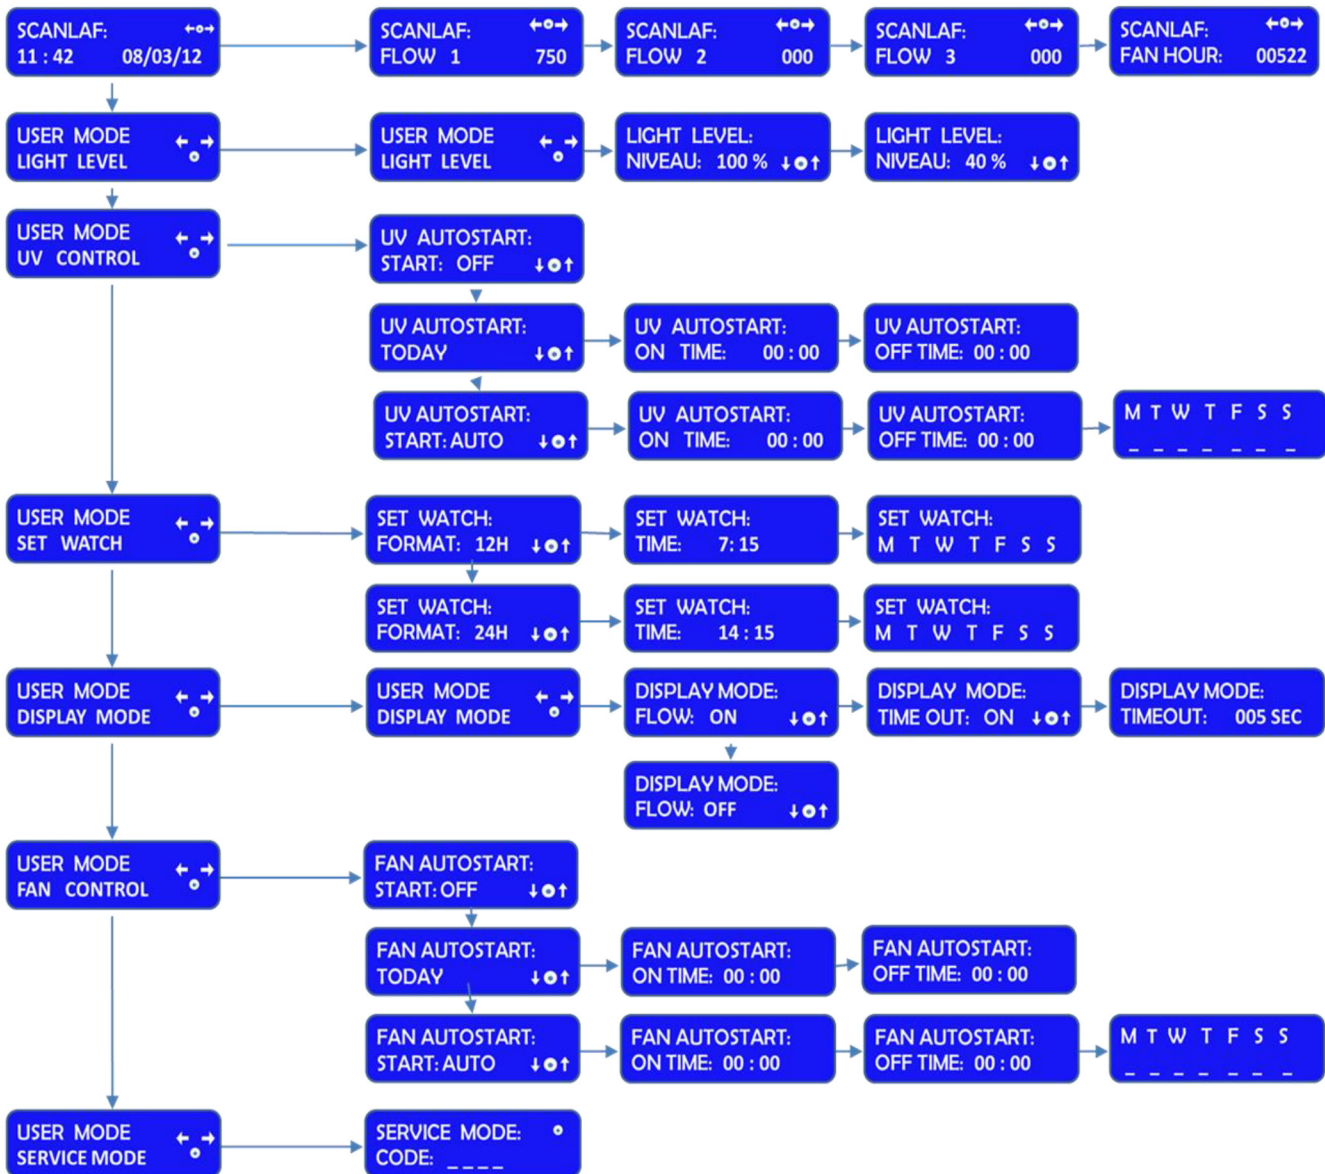

General air flow information & counter


This section describes how to access information about the running hours of the fan. The fans are designated FLOW 1, FLOW 2.



To learn how to enable and disable these functions refer to the section “Programming the Air Flow to Auto Start”.




Standard display



SCANLAF: ←→
FLOW 1 750

Press the right or left arrow button to navigate towards the FLOW information.


SCANLAF with FLOW 1 will be displayed together with a value. This value is for internal service information.



SCANLAF: ←→
FLOW 2 000

Press the right or left arrow button to navigate towards the FLOW information.


SCANLAF with FLOW 2 will be displayed together with a value. This value is for internal service information.



SCANLAF: ←→
FLOW 3 000

Press the right or left arrow button to navigate towards the FLOW information.

SCANLAF with FLOW 3 will be displayed together with a value. This value is for internal service information.



SCANLAF: ←→
FAN HOUR: 00522

Press the right or left arrow button to navigate towards the FLOW information.

SCANLAF with FAN HOUR will be displayed together with a value. This value is the number of hours the fan has been running.

Adjusting the level intensity of the internal light

This section covers how to adjust the light intensity of the internal light of the workstation.

SCANLAF: ←→
11 : 42 08/03/12

Standard display



Press the “enter” button to enter the menu.

USER MODE ←→
LIGHT LEVEL ○

The USER MODE with the “LIGHT LEVEL” will be displayed together with a representation of the “Control & Programming Keys”. The first line with the arrow symbol “ ←→ ” enables the user to go back to the previous menu or to move to another function. The symbol “○” represents the “ENTER” button.



Press the “enter” button to validate your choice.

LIGHT LEVEL: ↓○↑
NIVEAU: 100 %

The LIGHT LEVEL and “NIVEAU: 100 % will be displayed together with a representation of the Control & Programming Keys



Press the up or down arrow. The level of intensity will go up or down. Repeat pressing the arrow until you reach the level of intensity desired. If you hold down the arrow, the light intensity will change more rapidly.




Press the “enter” button to validate and to return to the MENU or wait a few seconds and the display will return by itself to the standard display

Programming and Controlling the UV light timer


This section describes how to program the UV light timer.




Note: For this feature to work correctly, you must set up the date and time first. This is described in the section “Programming Time and Date”



Unintended UV Radiation will harm eyes and skin. For protection, use the timer to start the UV decontamination when not present in the workstation area. Use the front shield cover (optional) to contain the radiation.



Standard display



Press the “enter” button to enter the menu.

Press on the right arrow button to enter the next menu.




The USER MODE with the “UV CONTROL” will be displayed together with a representation of the “Control & Programming Keys. The first line with the arrows symbol “◀ ▶” enables the user to go back to the previous menu or to move to another function. The symbol “o” represents the “enter” button.



Press the “enter” button to validate your choice.



The UV AUTOSTART with START: OFF will be displayed.



Press the up or down arrow to change the settings between START: OFF, TODAY and START: AUTO.



If you wish to program the UV light to start today, use UV AUTOSTART TODAY.



If you wish to program the UV light to start on a different day, use UV AUTOSTART START: AUTO.

UV Autostart Option Selected: “TODAY”



Press the “enter” button to enter the menu.



The UV AUTOSTART and “ON TIME: 00:00” will be displayed. This is the time at which the UV light should start



Press the “enter” button to validate your choice.



The first digit of the hour will be blinking. To enter the hour press the appropriate number found on the control panel. Continue this operation for the hours and the minutes. This will indicate the Time when the UV Light will switch ON automatically.



Press the “enter” button to validate your choice.

UV AUTOSTART:
OFF TIME: 00 : 00

The UV AUTOSTART and “OFF TIME: 00:00” will be displayed. This is the Time at which the UV Light will switch off.



Press the “enter” button to validate your choice.

UV AUTOSTART:
OFF TIME: 0 : 00

The first digit of the hour will be blinking. To enter the hour press the appropriate number found on the control panel. Continue this operation for the hours and the minutes. This will indicate the time when the UV light will turn OFF automatically.



Press the “enter” button to validate your choice.

UV Autostart Option Selected: “AUTO”



Note: For this feature to work correctly, you must set up the date and time first. How to do this is described in the section “Programming Time and Date”



Press the “enter” button to enter the menu.

UV AUTOSTART:
ON TIME: 00 : 00

The UV AUTOSTART and “ON TIME: 00:00” will be displayed. This is the time at which the UV light should start.



Press the “enter” button to validate your choice.

UV AUTOSTART:
ON TIME: 0 : 00

The first digit of the hour will be blinking. To enter the hour press the appropriate number found on the control panel. Continue this operation for the hours and the minutes. This will indicate the time when the UV Light will switch ON automatically.



Press the “enter” button to validate your choice.

UV AUTOSTART:
OFF TIME: 00 : 00

The UV AUTOSTART and “OFF TIME: 00:00” will be displayed. This is the Time at which the UV Light will switch off.



Press the “enter” button to validate your choice.

UV AUTOSTART:
OFF TIME: 0 : 00

The first digit of the hour will be blinking. To enter the hour press the appropriate number found on the control panel. Continue this operation for the hours and the minutes. This will indicate the time when the UV light will turn OFF automatically.



Press the “enter” button to validate your choice.

M T W T F S S


The Week display will appear “ M T W T F S S ”



Press the “enter” button to validate your choice.

M T W T F S S
█ - - - - -

The Monday option will be blinking.

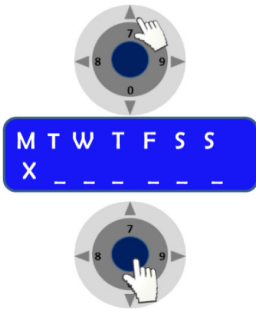


Press on the UP arrow to select Monday. Press the right and left arrows to navigate between the days,

In this example the Monday option will be marked with an "X" to indicate that the UV light will be ON on Monday at the desired time and will be switched OFF at the desired time programmed earlier in this section.

Press on the "enter" button to confirm

Programming Time and Date

This section describes how to set the time and the date.

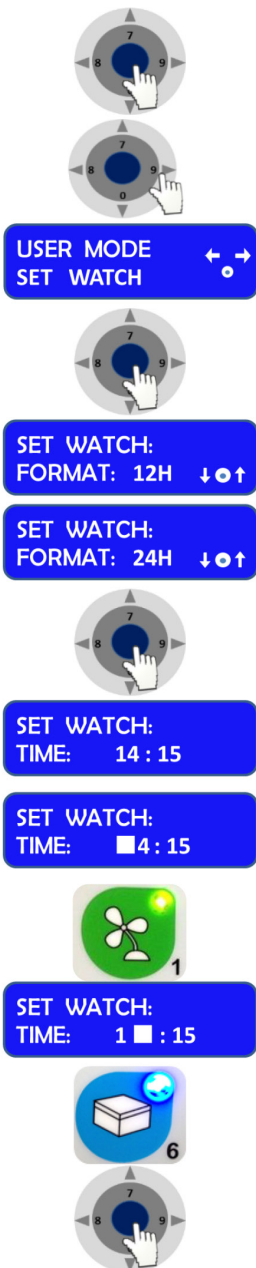

Press the "enter" button to enter the menu.

Press the right or left arrow button to reach the menu displaying "SET WATCH".

The USER MODE menu with SET WATCH will be displayed together with a representation of the "Control & Programming keys".

Press the "enter" button to enter the menu.

The SET WATCH menu with FORMAT: 12H or 24H will be displayed together with a representation of the "Control & Programming keys"

Press on the DOWN or UP arrows to change the settings from 12H to 24H and vice versa.

Press the "enter" button to enter the menu.

The SET WATCH menu with TIME will be displayed.

The first digit of the hour will be blinking. To enter the hour press the appropriate number found on the control panel.

Example: Setting up the watch at 16:39

Press the button that has the number 1 and it will be registered on the display.

The second digit of the hour will be blinking.

Press the button that has the number 6 and it will be registered on the display. Continue this to fill out all digits.

Press the "enter" button to enter the menu, and press the right or left arrow buttons to reach the menu displaying "SET WATCH"

SET WATCH:
M T W T F S S

The SET WACH menu with the day's first letter "M T W T F S S" will be displayed.

SET WATCH:
M ■ W T F S S


Press on the RIGHT or LEFT arrow button to navigate to the correct day.



Press the "enter" button to validate your choice.

SET WATCH:
DATE: 13 / 03 / 12

The SET WACH menu with DATE will be displayed. The Date has the format of DD / MM/ YY.




Press the RIGHT arrow button to navigate to the day, month or year section. Use the same method for setting the time to enter the date.

Programming the Air Flow to auto start (Weekly or Daily)

This section describes how to enable and program the airflow to auto start on a specific date and time, and how to disable that feature.



Press the "enter" button to enter the menu.



Press the RIGHT or LEFT arrow button to reach the menu displaying "FAN CONTROL"

USER MODE
FAN CONTROL


The USER MODE menu with FAN CONTROL will be displayed together with a representation of the "Control & Programming Keys."



Press the "ENTER" button to enter the menu.

FAN AUTOSTART:
START: OFF

The FAN AUTOSTART and "START: OFF" will be displayed. This indicates that the auto start function is disabled.



Press Down or UP to change the settings. Two options can be selected FAN AUTOSTART: TODAY, or, FAN AUTOSTART: START:AUTO.:


FAN AUTOSTART:
TODAY

The FAN AUTOSTART and "TODAY" indicate the auto start function can be programmed for the current day at a specific time.

FAN AUTOSTART:
START: AUTO

The FAN AUTOSTART and "START: AUTO" indicate the auto start function can be programmed any given day and time.

Option selected: TODAY



Press the "enter" button to enter the menu.

FAN AUTOSTART:
ON TIME: 00 : 00



The FAN AUTOSTART and “ON TIME: 00:00” will be displayed. This is the time at which the fans should start.

Press the “enter” button to enter the menu.

FAN AUTOSTART:
ON TIME: ■0 : 00



The first digit of the hour will be blinking. To enter the hour press the appropriate number found on the control panel. Continue this operation for the hours and the minutes. This will indicate the time when the fan will turn ON automatically.

Press the “enter” button to validate your choices.

FAN AUTOSTART:
OFF TIME: 00 : 00



The FAN AUTOSTART and “OFF TIME: 00:00” will be displayed. This is the time at which the fans will turn off.

Press the “enter” button to enter the menu.

FAN AUTOSTART:
OFF TIME: ■0 : 00



The first digit of the hour will be blinking. To enter the hour press the appropriate number found on the control panel. Continue this operation for the hours and the minutes. This will indicate the time when the fan will turn OFF automatically.

Press the “enter” button to confirm your choices.

Option selected: AUTO



Note: For this feature to work correctly, you must set up the date and time first. How to do this is described in the section “Programming Time and Date”



Press the “enter” button to enter the menu.

FAN AUTOSTART:
ON TIME: 00 : 00



The FAN AUTOSTART and “ON TIME: 00:00” will be displayed. This is the time at which the fans should start.

Press the “enter” button to enter the menu.

FAN AUTOSTART:
ON TIME: ■0 : 00



The first digit of the hour will be blinking. To enter the hour press the appropriate number found on the control panel. Continue this operation for the hours and the minutes. This will indicate the time when the fan will turn ON automatically.

Press the “enter” button to validate your choices.

FAN AUTOSTART:
OFF TIME: 00 : 00

The FAN AUTOSTART and “OFF TIME: 00:00” will be displayed. This is the time at which the fans will turn off.



Press the “enter” button to enter the menu.

FAN AUTOSTART:
OFF TIME: 0 : 00

The first digit of the hour will be blinking. To enter the hour press the appropriate number found on the control panel. Continue this operation for the hours and the minutes. This will indicate the time when the fan will turn OFF automatically.



Press the “enter” button to confirm your choices.

M T W T F S S
- - - - -

The Week display will appear “ M T W T F S S”



Press the “enter” button to validate your choice.

M T W T F S S
■ - - - -

The Monday option will be blinking.



Press on the UP arrow to select Monday or press the right and left arrows to navigate between the days,

M T W T F S S
X - - - -

In this example the Monday option will be marked with an “X” to indicate that the fan will be ON, on Monday at the desired time and will be switched OFF at the desired time programmed earlier in this section.




Press on the “enter” button to confirm

Display Mode Functions

This section describes how to enable and disable the Flow and Fan information presented in the overview of the control panel menu.



Press the “enter” button to enter the menu.



Press the RIGHT or LEFT arrow button to reach the menu displaying “DISPLAY MODE”

USER MODE
DISPLAY MODE ← →

The USER MODE menu with DISPLAY MODE will be displayed together with a representation of the “Control & Programming Keys”.



Press the “enter” button to enter the menu.

DISPLAY MODE:
FLOW: ON ↓ ● ↑

The DISPLAY MODE and “FLOW: ON” will be displayed together with a representation of the Control & Programming Keys.




Press the up or down arrow to select the between up or on mode. This feature will disable the view of the information on FLOW 1, FLOW 2 AND FLOW 3



Press Enter to validate. The display will return to DISPLAY MODE.



Press the “enter” button to enter the menu.



Press the DOWN or UP arrow to reach the following display:




The DISPLAY MODE and “TIME OUT” will be displayed together with a representation of the Control & Programming Keys.



Press the “ENTER” button to enter the menu to turn this function ON or OFF. Turning this function OFF will disable the following display and return to DISPLAY MODE.



Press the “enter” button to enter the menu.



Press on the DOWN or UP arrow to reach the following display:



The DISPLAY MODE and “TIME OUT: 005 SEC” will be displayed. This feature indicates that any information or changes will remain displayed for 5 seconds before returning to the Standard Display. The display time is of a minimum of 5 seconds and therefore can only be increased. To increase the duration of the displayed information use the UP and DOWN arrows.

HEATED SURFACE


The heated surface is only applicable on the TITAN IVF model.

The TITAN uses an electrical heating for the heated surface with PT 100 sensor

The heated area is indicated by a brushed steel effect in the work surface.

Operational Characteristics

The heated surfaces, will be heated to 37°C, and are controlled by an accurate sensor and a control processor.

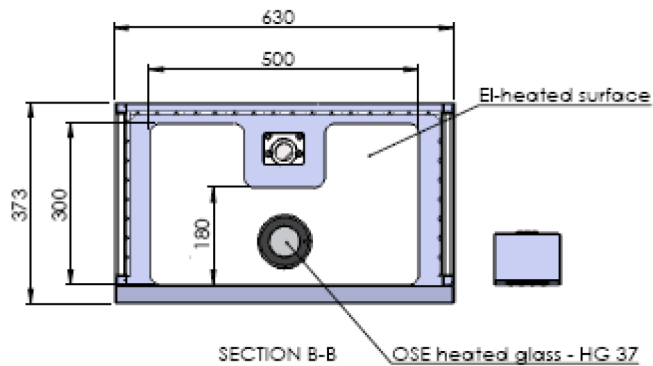

Placing of large hot or cold masses on the heated elements will affect the regulation process and should be avoided during normal operation.


Placing a hand will also draw heat from the surface, therefore please avoid placing fingers or a hand on the surface during warming up or during the calibration of the controller.

Turn on the heating system for at least 60 minutes before starting the work. If possible, place all needed equipment on the surface during the warming up period to warm these appropriately. Always wait for the temperature to stabilize completely before starting work.



CAUTION. There is heat loss from the edges of the heated surface. Do not place temperature sensitive material there.

Temperature Controller

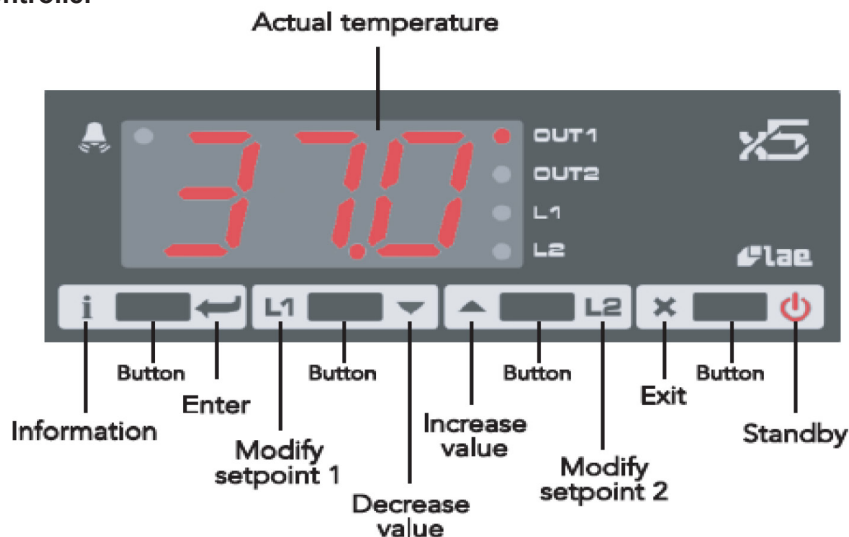

The display shows the temperature readout from the chosen channel (only channel 1 is used in this example). In case of an alarm situation, a red light will start flashing in the top left-hand corner of the display. On the right-hand side of the display, an indication of parameter can be viewed. Below lists all possible values and messages that can be shown in the display:

Display	Description
OFF	Controller is in standby
OR	Probe T1 out of range or failure
HI	Room high temperature alarm
LO	Room low temperature alarm
TUN	Controller is in auto tuning
E1	In tuning: Timeout 1 error
E2	In tuning : Timeout 2 error
E3	Out of range error
LED	Description
OUT1	Channel 1 output
OUT2	Channel 2 output
L1	Channel 1 set point modification
L2	Channel 2 set point modification
	Alarm
Information	Description
THI	Maximum temperature recorded
TLO	Minimum temperature recorded
LOC	Keypad state lock





The four buttons for operating the temperature controller are placed below the display. These are described in the figure above.

Each button has two functions - one on each side of the button. Simply press the appropriate symbol to use the buttons.

The heated surface is designed to provide and maintain a constant 37 °C over the heated part of the working surface to within ± 0.2 °C at a maximum ambient temperature of 35 °C. The controller is operating in PID (Proportional-Integral-Derivative) mode to get the most accurate and stable temperature possible.

User Setup




The units are delivered ready for use from the factory. Below is the process to access the parameters in the temperature controller.

Button	Description
	Show value
	Select data by using the up and down arrows
	Enter
	Exit the menu






Note: After 10 seconds without activity, the menu will exit.




Accessing the parameters and information menu

-  Press and release the information button.
-  To the select the data to be displayed press the UP or DOWN arrow.
-  Press the information button to display the value you have selected.

Resetting the THI and TLO recordings

-  To the select the data to be reset press the UP or DOWN arrow.
-  Press the information button to display the value you have selected.
-  To reset the value, press and hold the information button simultaneously with the exit button.

Channel 1 set point

-  Press and release L1. The LED L1 will flash and the display will show 1SP (set point) for 1 second and then the set point associated value.
-  To select the desired value press the UP or DOWN arrow.
-  To store the desired value press enter or wait 10 seconds



To reset the value, press and hold the information button simultaneously with the exit button.

Standby

This section describes how to put the controller on standby, or resume from standby.



Press down the standby button for 3 seconds.

Keypad lock

The keypad lock can be used to protect the settings from intentional or unintentional changes.



Press the information button to enter the INFO menu.

Use the UP and DOWN arrows to select LOC (keypad lock). Set the parameter LOC = YES to lock the keypad.

To unlock the keypad, change the setting to LOC = NO.

Operating the heated areas

Normal Operation

The temperature controller will maintain the work surface temperature at 37 °C and will not require any user interaction after the initial setup performed by a service technician.

Checking the temperature

The actual temperature of the surface is shown on the display (OUT1). L1 will show the set point temperature.

TROUBLESHOOTING YOUR WORKSTATION

Flow 1 alarm




You have an alarm on the FLOW 1. This indicates that a calibration of the inflow and downflow is needed.

Before starting, make sure the window is lowered to its normal working height. Make sure that all accessories, devices regularly used in the workstation are in place and not taken out. Then follow the instructions



From STANDARD DISPLAY




Press the RIGHT or LEFT arrow button to navigate towards the Information menu until you reach the SERVICE MODE.



Press the "ENTER" button to enter the service functions



Enter code 1234 using the numbers found on the control panel and press enter.



Press on the RIGHT or LEFT arrow button to navigate towards the Information menu until you reach the FLOW SENSORS menu.



Press on the "ENTER" button



FLOW SENSOR 1 with as a standard type ANALOG is displayed. If not SWITCH will be displayed. FLOW SENSOR 1 is the down flow.



Press on the "ENTER" button.




NEW CALIBRATION will be displayed.



Press on the "ENTER" button



FLOW ALARM 1 with HIGH and a set of values will be displayed (e.g. 0285)



Press the arrow down until the alarms starts. By pushing the arrow the numbers will decrease by units.



By maintaining a constant pressure on the arrow, the numbers will decrease by decimals.



Press the arrow up one unit at a time and wait for 2 to 3 seconds to see if the alarm stops.



Repeat the operation until the alarm stops.



When the alarm has stopped, read the value displayed: e.g. 0225. Add 50 to the number: $0225 + 50 = 0275$. Press on the arrow up until you reach this number.



Press on the "ENTER" button.



FLOW ALARM 1 with LOW and a set of values will be displayed (e.g. 0175)



Press the arrow up until the alarms starts. By pushing the arrow the numbers will decrease by units.



By maintaining a constant pressure on the arrow, the numbers will decrease by decimals.



Press the arrow down one unit at a time and wait for 2 to 3 seconds to see if the alarm stops.



Repeat the operation until the alarm stops.



When the alarm has stopped, read the value displayed: e.g. 0125. Add 50 to the number: $0125 + 50 = 0175$. Press on the arrow down until you reach this number.



Press on the "ENTER" button.



FLOW ALARM 1 with ALARM NORMAL will be displayed.



Press the "ENTER" button.



FLOW SENSOR 2 with a standard type ANALOG will be displayed. If not, SWITCH will be displayed. FLOW SENSOR 2 is the Inflow/ exhaust.



Press the “ENTER” button




NEW CALIBRATION will be displayed.



Press the “ENTER” button.



FLOW ALARM 2 with HIGH and a set of values will be displayed. (e.g. 0305)



Press the arrow down until the alarms starts. By pushing the arrow, the numbers will decrease by units.



By maintaining a constant pressure on the arrow, the numbers will decrease by decimals.



Press the arrow up one unit at a time and wait for 2 to 3 seconds to see if the alarm stops.



Repeat the operation until the alarm stops.



When the alarm has stopped, read the value displayed: e.g. 0225. Add 50 to the number: $0225 + 50 = 0275$. Press on the arrow up until you reach this number.



Press the “ENTER” button.



FLOW ALARM 1 with LOW and a set of values will be displayed. (e.g. 0205)



Press the arrow up until the alarms starts. By pushing the arrow the numbers will decrease by units.



By maintaining a constant pressure on the arrow, the numbers will decrease by decimals.



Press the arrow down one unit at a time and wait for 2 to 3 seconds to see if the alarm stops.



Repeat the operation until the alarm stops.



When the alarm has stopped, read the value displayed: e.g. 0125. Add 50 to the number: $0125 + 50 = 0175$. Press on the arrow down until you reach this number.



Press the “ENTER” button.

FLOW ALARM 2:
ALARM: NORMAL ↓○↑

FLOW ALARM 1 with ALARM NORMAL will be displayed.



Press the “ENTER” button.

FLOW SESNSOR 3 :
TYPE: NONE ↓○↑

FLOW SENSOR3 with TYPE NONE is displayed.



Press the “ENTER” button and navigate in the menu until your reach SERVICE LOGOUT.


SERVICE:
LOGOUT ←○→

Press the “ENTER” to LOGOUT and reach the Standard Display.



TECHNICAL SPECIFICATIONS

TITAN IVF and TITAN LAF

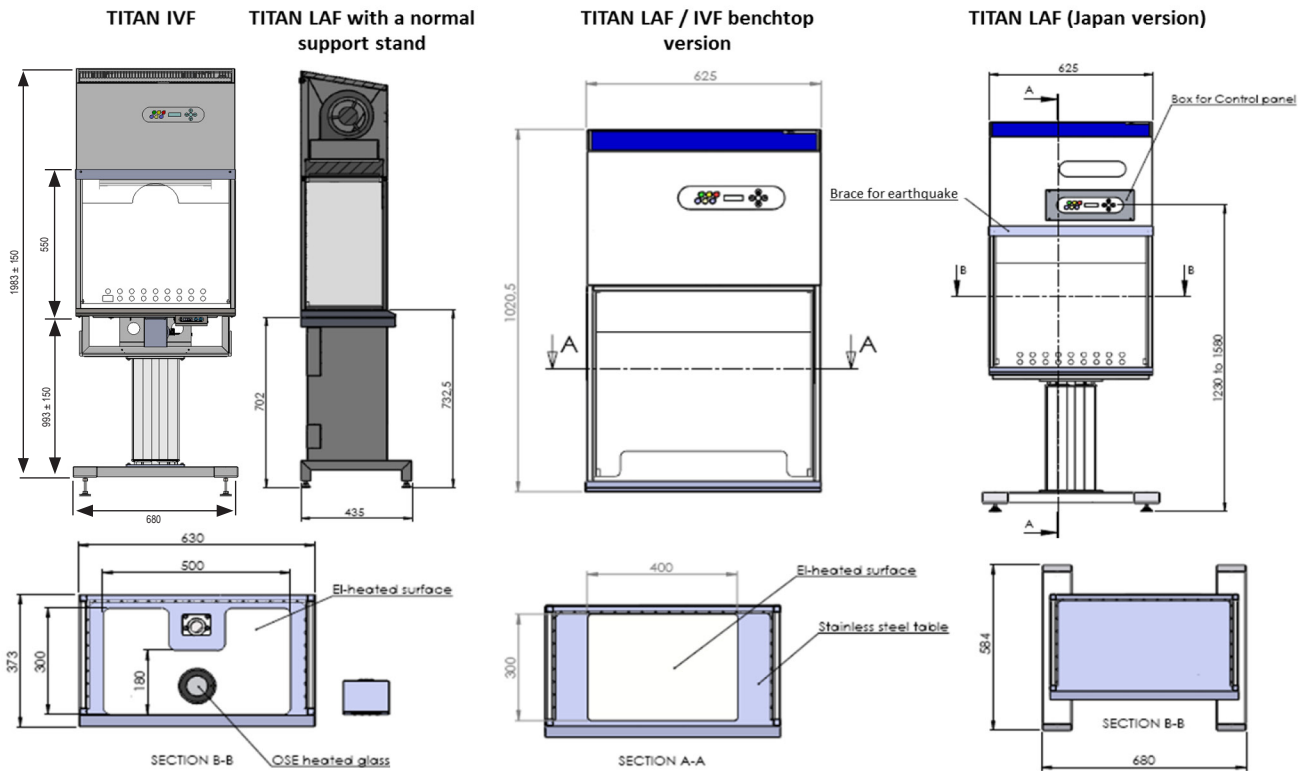

TITAN IVF/LAF

TITAN IVF Dimensions (W x D x H) with adj. Height	630 X 584 x 1983 (+/-150) mm
TITAN LAF / IVF benchtop version (W x D x H)	630 x 340 x 1020 mm
Table plate dimensions (W x D)	573 x 318 mm
TITAN IVF Heated surface dimensions (W X D)	500 x 300 mm
TITAN LAF With heated Surface dimensions (W x D)	400 x 300 mm
Air velocity, vertical flow	0,28 m/s (adjustable 0.01 -0.70 m/s)
Air Velocity, deviation	+/- 10%
Noise Level, ISO 6081	<50 dB(A)
Light intensity variable	0 – 700 Lux
HEPA Filters, EN 1822	Efficiency is 99.999% against 0.3 µm particle H-14 size
Energy consumption	0,2 A
Fuses	10 A
Voltage / Frequency	220-240V / 50-60 Hz or 110 -120V / 50 -60 Hz
Window material (side/Front)	Laminated safety glass
Cabinet material / Work surface	Polyester coated steel /AISI 304 stainless steel
Packing Dimensions (W x D x H)	916 x 716 x 1559 mm
Shipping volume	1,03 m³
Net Weight / Gross Weight	131 Kg / 171 Kg

SPARE PARTS

Contact Customer Service for any information regarding spare parts. Contact information is located on the last page of this document.

OPERATING THE STEREO MICROSCOPE HEATED GLASS AND LIGHT SOURCE CONTROLLER

Overview of Unit

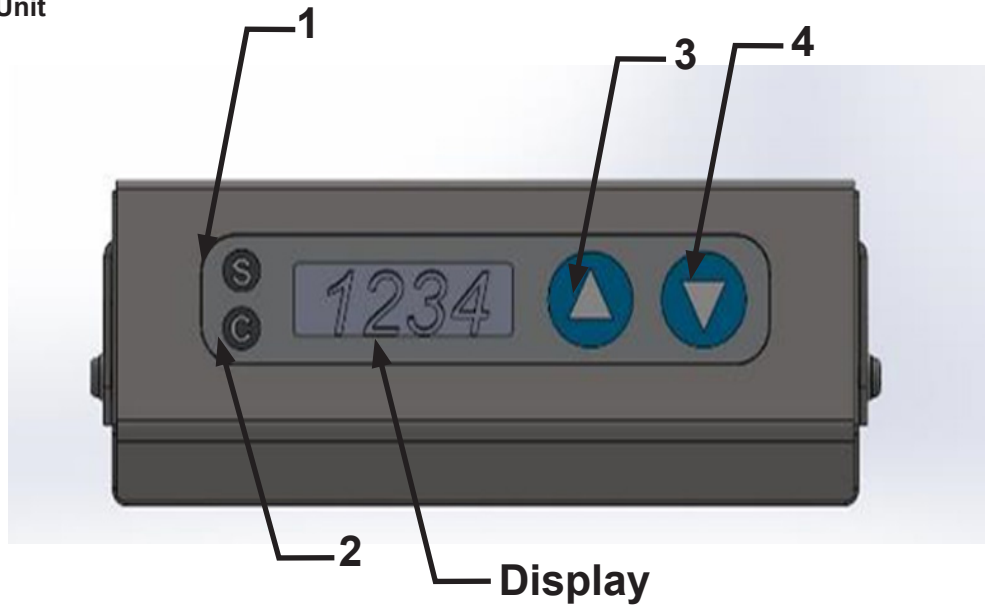


Figure 1 Heated Glass and Light Source controller seen from front

1	“S” Push button for Set-point mode
2	“C” Push button for Calibration mode
3	“Arrow Up” Push button to increase light-intensity or temperature in Set point mode or temperature in Calibration mode
4	“Arrow Down” Push button to decrease light intensity or temperature in Set point mode or temperature in Calibration mode
Display	Display to indicate temperature on Heated glass

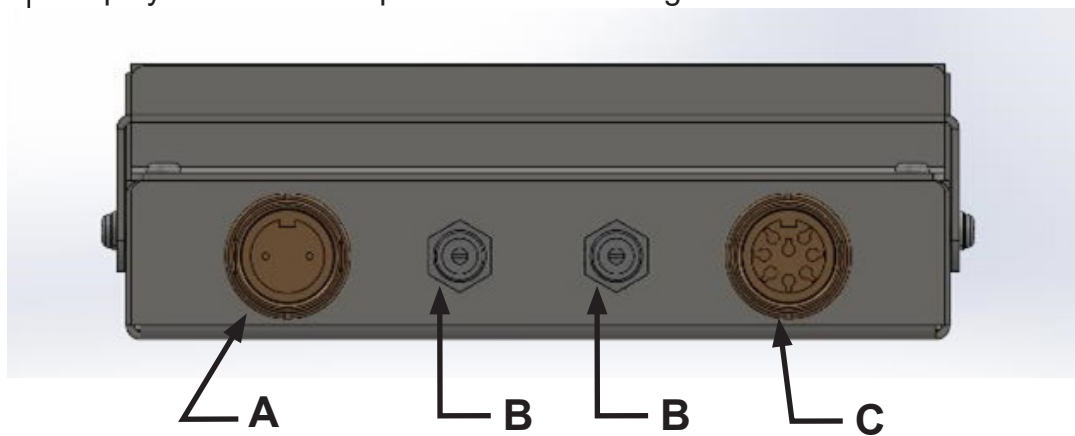


Figure 2 Rear view of controller for Heated glass and Light source

A	Connector for LS112 light source
B	Connector for Power input or Power output
C	Connector for Heated glass

Installation

CAUTION: Only a person from Origio or a person authorized by Origio should install the units

The HG/LS controller must be attached to the stainless steel studs under the table top of the Origio Fortuna workstation as shown below.

Position the LS 112 Light Source under the Workstation tabletop with the lamp house pointing toward the rear of the Workstation.

Fasten the LS112 Light Source under the Workstation table plate as shown, using the finger nuts provided. Be sure that the light source is in level and nuts are fastened

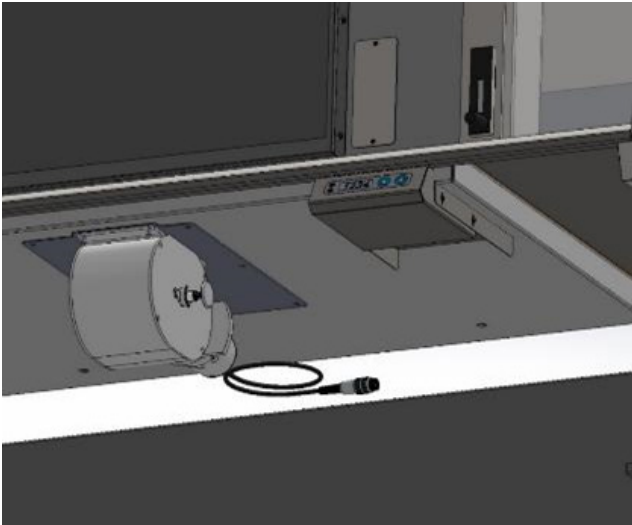


Figure 3 HG/LS controller installed in workstation with 1 workplace

For workstations with a single workplace the HG/LS controller is supplied as configuration a) and mounted as shown in figure 3

In workstations with dual workplaces 2 HG/LS controllers are supplied. One is supplied as configuration a) and one as configuration b). In this case the HG/LS controller are mounted, with one in left and one in right side.

Cable from the Light source is connected to A as shown in figure 2.

Cable from Heated glass is connected to C as shown in figure 2.

In workstations with a single workplace, the connection from the power supply is connected to one of the B connectors as shown in figure 2.

In workstations with dual workplaces, the power supply is connected to one of the B connectors as shown in figure 2 and the power extension cable is connected from the other B connector to one of the B connectors on the other HG/LS controller.

Operation

Mode	User Interactions
Normal mode (Default)	Control of light intensity and turn Heated Glass ON and OFF
Set-Point mode	Change desired temperature on heated glass
Calibration mode	Calibrate the temperature sensor in the heated glass

The 3 modes are described below

Normal Mode

A special heat indicator can be seen in the heated glass as shown in Figure 4.

When the workstation is powered up the indicator, the heated glass will always be switched on. The indicator will turn red as shown.

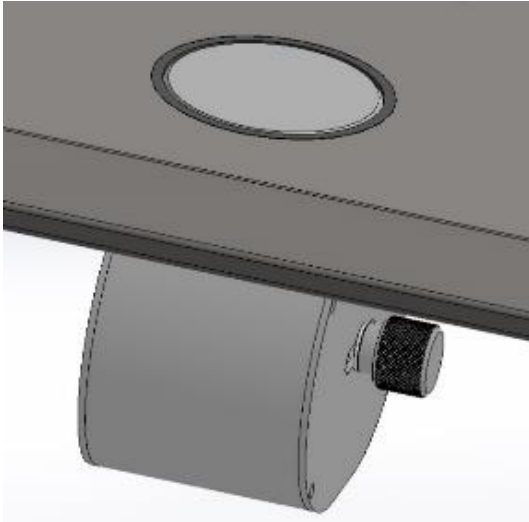


Figure 4 Heated glass outside temperature limits

The Display will start at room temperature and increase until it reaches the setpoint. If the setpoint is 37.0C the temperature will increase until the display shows 37.0 as shown in Figure 5



Figure 5 Display in Normal mode (IVF versions)

When the setpoint is reached the indicator in the heated glass will change to green.

The indicator will stay green when the temperature is at setpoint +/- 0.50C, when outside the range the indicator will shift to red to warn the user.


Light Source control in normal mode

It is possible in normal mode, to switch microscope light source on and off as well as changing intensity of the light. The light can be adjusted in 30 levels.

See location of buttons in Figure 1

Increase light	Press or hold "Arrow Up"
Decrease light	Press or hold "Arrow down"
Turn light off	Press "Arrow up" and "Arrow down" simultaneously
Turn light on	Press "Arrow up" or "Arrow down" Light intensity is the same as last time the light was turned off

When increasing light level, the display shows the actual light level for 1 second. Below is the display shown at light level 10. After 1 second, the display changes to show the temperature

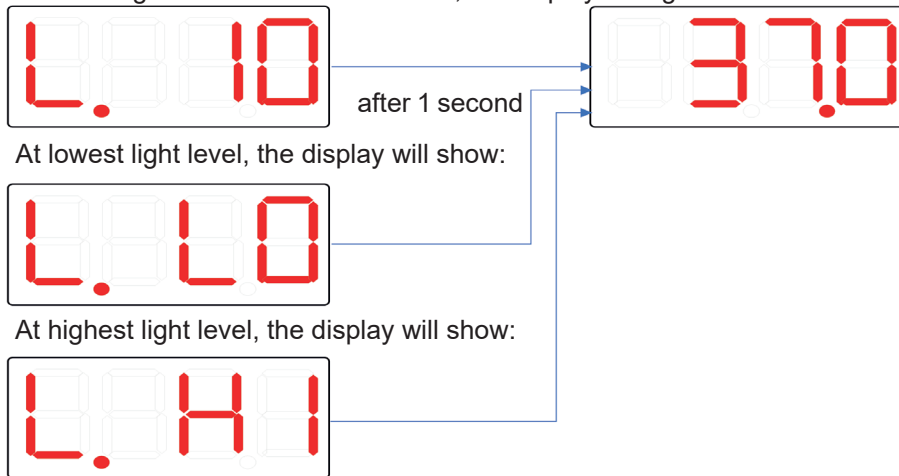

The Controller will remember last light level after power down and power up again.



The knob for adjusting the mirror is placed on the left hand side of the Light Source. The rotatable mirror has two different sides. One side is a plane mirror, while the other is concave.


The plane mirror is used when a high magnification is needed and the concave mirror is used for when lower magnification is needed. Virtual dark field is obtained by positioning the mirror almost vertically. The mirror can be rotated 360 degrees in a rotational pattern and moved 45 mm horizontally, which enables positioning for an optimal lightning of the object.

Turn the Heated glass on and off in normal mode.


It is possible to turn the Heated glass of by holding the “S” button pressed for 3 seconds. When the heated glass has been turned off the display will show



The indicator in the Heated glass will slowly fade between red and green to indicate that the Heated glass has been turned off.



To turn the Heated glass on again, hold the “S” button pressed for 3 seconds. The display will show the following for 1 second and then return to show temperature



Heated Glass Set point mode

To enter set-point mode hold the “S”, “Arrow Up” and “Arrow Down” buttons pressed for 1 second simultaneously. A flashing S indicates that the controller is in Set-point mode.

The Display will show the last chosen set-point. For instance, 37.0 as shown in Figure 6. To change desired temperature up or down, press the “Arrow up” or “Arrow down” several times, or hold it in, until the desired temperature has been reached.



Figure 6 Flashing Display in Set Point Mode

Leave the Set-point mode by pressing the “S” once. The Display will return to normal mode.

Heated Glass Calibration Mode

CAUTION: Calibration of the sensor in the heated glass requires a reference thermometer with a special probe, such as the F100 Thermometer, Origio order no: 11010, together with the Solid Temperature sensor Origio order no: 11006.

Place the Solid temperature sensor on the heated glass, turn on the F100 instrument. Wait 10 min until the temperature reading in the Thermometer has stabilized.

- a.) To enter calibration mode, hold the “C”, “Arrow Up” and “Arrow Down” buttons pressed for 1 second simultaneously. A flashing c indicates that the controller is in calibration mode.
- b.) The Display will show the temperature assumed by the controller. For example, refer to Figure 7.





Figure 7 Flashing Display in Calibration mode

- c.) Leave the Calibration mode by pressing the “C” once. The Display will return to normal mode.
- d.) Wait 10 min or until the display on the F100 thermometer has stabilized. Read the actual temperature on the Thermometer. If necessary, repeat the calibration from a).

The LS112 can be supplied with filters for specific light conditions.

1. No filter inserted (included)
2. Green filter
3. Red filter
4. Blue filter



OPERATING THE LCD MONITOR



Depending on the customer order and the configuration selected, please refer to the User manual provided with the monitor.

WARRANTY AND LIABILITY

Limited Warranty

ORIGIO Equipment warrants to the purchasers of all devices and products solely manufactured by ORIGIO EQUIPMENT.

In the event of product failure under normal use, due to defects in material or workmanship, within a period of twenty four months (24) months from the date of invoice of the Product and from the point of origin, the product will be repaired, or at ORIGIO EQUIPMENT option, replaced, at no charge. ORIGIO EQUIPMENT assumes that the Purchaser is experienced in the use of this device and is able to judge from his/her own expertise the suitability or otherwise of the product for the intended use. This limited warranty does not apply to products subjected to abnormal use or conditions, improper storage, damaged by accident, misuse or abuse, improper line voltage, products whose serial number has been altered, to products not shipped in accordance with the recommendations of ORIGIO EQUIPMENT , and/or to products altered or serviced by anyone other than ORIGIO EQUIPMENT authorized distributors. Distributor is responsible for the labor and travel costs during this period.

This limited warranty is exclusive and in lieu of all other warranties whether written, oral, expressed or implied. In particular, ORIGIO EQUIPMENT does not warrant that the product is suitable for the needs of the purchaser and there are no warranties given as to merchantability or fitness for a particular purpose other than the one specified in ORIGIO EQUIPMENT literature that accompanies every specific product.

ORIGIO EQUIPMENT reserves the right to change or discontinue this product without prior notice.

Liability:

Because ORIGIO EQUIPMENT has no control or influence over the conditions under which this device is used, over its method of use or administration, or on handling of the product after it leaves its possession ORIGIO EQUIPMENT takes no responsibility for the results, use and/or performance of the product. ORIGIO EQUIPMENT expects that use of the product will be confined to trained and expert users.

In no event shall ORIGIO EQUIPMENT be liable for any direct or indirect damages including incidental, consequential or special damages, arising out of or in connection with the use or performance of the product.

If ORIGIO EQUIPMENT provides you with technical documentation, this does not authorize you to perform repairs, adjustments or alterations on the device or accessories.

No representative of ORIGIO EQUIPMENT and no vendor of the product is authorized to change any of the foregoing terms and conditions, and the purchaser accepts the product subject to all terms and conditions herein, subject always to any contrary provisions which are necessarily implied by stature or law notwithstanding the within terms and conditions.

Replacement

As mentioned in the Limited Warranty, The decision whether to provide any remedy or whether to refund any portion of the purchase price shall be at the discretion of ORIGIO EQUIPMENT.

Before returning a product for any reason, please contact your nearest ORIGIO EQUIPMENT distributor for assistance and instructions.

CUSTOMER SERVICE CONTACT INFORMATION

ORIGIO a/s Knardrupvej 2
2760 Måløv
Denmark
Tel: +45 46 79 02 00
Fax: +45 46 79 03 00
Customer.service@origio.com
www.origio.com

CooperSurgical, Inc.
95 Corporate Drive
Trumbull, CT 06611 USA
Phone: (800) 243-2974
Fax: (800) 262-0105
International
Phone: +1 (203) 601-9810
Fax: +1 (203) 601-4747
service@origio.us.com



Made in Lithuania



CooperSurgical, Inc.
95 Corporate Drive
Trumbull, CT 06611 USA
Phone: (800) 243-2974
Fax (800) 262-0105
www.coopersurgical.com

International
Phone: +1 (203) 601-9818
Fax +1 (203) 601-4747

UK Responsible Person
Research Instruments Ltd
Bickland Industrial Park,
Falmouth, Cornwall TR11 4TA, UK