

PVP Clinical Grade

Product No.:

1090

Customer Service:

E-mail: sales@coopersurgical.com



ORIGIO a/s

Knardrupvej 2, 2760 Måløv, Denmark

www.fertility.coopersurgical.com

Tel: +45 46 79 02 00

Sponsor: ORIGIO AUSTRALASIA Pty Ltd

Level 3, Customs House

31 Alfred Street, Sydney, NSW 2000

Australia

origio

a CooperSurgical Company

Explanation of Symbols (in random order)



Indicates a medical device that is intended for one use, or for use on a single patient during a single procedure



Do not use if package is damaged



Discard excess (unused) media following warming



Indicates the medical device manufacturer



Indicates the manufacturer's batch code so that the batch or lot can be identified



Indicates the date after which the medical device is not to be used



Indicates the manufacturer's catalogue number so that the medical device can be identified



Indicates a medical device that has been manufactured using accepted aseptic techniques




Indicates a medical device that needs protection from light sources





Indicates the need for the user to consult the instructions for use



Indicates the need for the user to consult the instructions for use for important cautionary information such as warnings and precautions



Indicates the temperature limits to which the medical device can be safely exposed

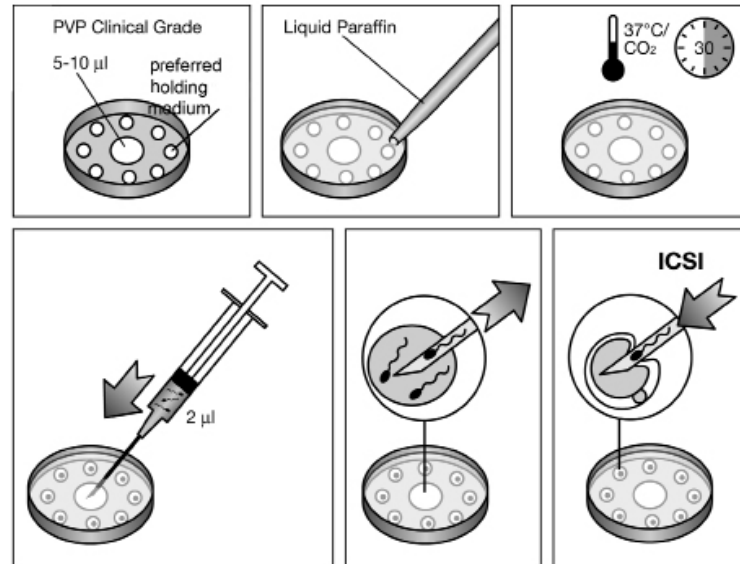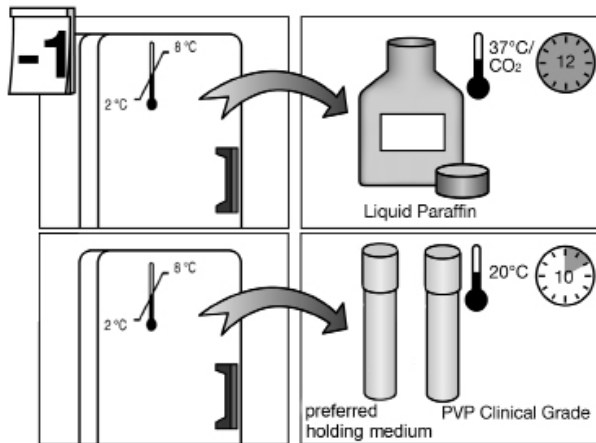

PVP Clinical Grade

Intended use

PVP Clinical Grade is used for slowing down the movement of the spermatozoa for ICSI.

This product is for ART treatment, whether the cause of infertility is male or female. The product should only be used by professionals trained in ART treatment.

Composition

Synthetic Serum Replacement (SSR®)*

(USA: ART Supplement)

* Contains Recombinant Human Insulin

Human serum albumin (HSA)

Polyvinylpyrrolidone

Glucose

Sodium pyruvate

Physiological salts

Sodium bicarbonate

HEPES

Gentamicin sulphate 10µg/ml

Quality control testing

Sterility tested (Ph.Eur., USP)

Osmolality tested (Ph.Eur., USP)

pH tested (Ph.Eur., USP)

Endotoxin tested ≤ 0.2 EU/ml (Ph.Eur., USP)

Sperm Survival Test $\geq 80\%$

Sperm Immobilisation tested

Note: The results of each batch are stated on a Certificate of Analysis, which is available on www.fertility.coopersurgical.com

Storage instructions and stability

The products are aseptically processed and supplied sterile.

Store in original container at 2-8°C, protected from light.

When stored as directed by the manufacturer the product is stable until the expiry date shown on the vial label.

Do not freeze

The product is provided in vials intended for single use.

Excess (unused) media should be discarded.

Precautions and warnings

Do not use the product if:

1. Product packaging appears damaged or if the seal is broken.
2. Expiry date has been exceeded.

Caution: All blood products should be treated as potentially infectious. Source material from which this product was derived was found negative when tested for antibodies to HIV, HCV, and non-reactive for HBsAg, HCV RNA and HIV-1 RNA. No known test methods can offer assurance that products derived from human blood will not transmit infectious agents.

The potential risk of reproductive or developmental toxicity due to the use of ART media has not been determined and is still unknown.

Notes:

Dispose of the device in accordance with local regulations for disposal of medical devices.

Due to native physical characteristics of PVP, small variations in viscosity may occur between batches.

The presence of human serum albumin (HSA) may occasionally cause a small amount of precipitation in the medium.

Instructions for use

1. Remove PVP Clinical Grade and preferred holding medium from storage at 2-8 °C and leave at room temperature for 10 minutes.
2. Depending on the number of oocytes for injection, pipette a corresponding number of 10 µl droplets of preferred holding medium onto the bottom of the ICSI dish.
3. In the middle of the same dish place a 5-10 µl droplet of PVP Clinical Grade.
4. Cover with pre-equilibrated Liquid Paraffin and place the dish in a 5-6% CO₂ environment at 37°C for 30 minutes prior to use.
5. Introduce 2 µl of prepared and washed sperm to the droplet of PVP Clinical Grade. The PVP will reduce the motility of the sperm and facilitate the capture and loading of a single spermatozoon in the injection pipette.